



Amicon® Ultra-0.5 Centrifugal Filter Devices

for volumes up to 500 µL


User Guide




Fill



Spin



Recover



Collect

For research use only;
not for use in diagnostic procedures






Notice

The information in this document is subject to change without notice and should not be construed as a commitment by Millipore Corporation or an affiliated corporation. Neither Millipore Corporation nor any of its affiliated corporations assumes responsibility for any errors that may appear in this document. This manual is believed to be complete and accurate at the time of publication. In no event shall Millipore Corporation be liable for incidental or consequential damages in connection with or arising from the use of this manual.

© 2009 MILLIPORE CORPORATION. ALL RIGHTS RESERVED.

PR02725 Rev. B, 07/09

Millipore, Amicon, Centricon, Milli-Q, MultiScreen, and Ultracel are registered trademarks of Millipore Corporation.
The M mark is a trademark of Millipore Corporation.
Alconox and Terg-A-Zyme are registered trademarks of Alconox, Inc.
Lubrol is a registered trademark of Imperial Chemical Industries PLC.
Nonidet is a trademark of Royal Dutch/Shell Group.
Triton is a registered trademark of Union Carbide Corporation.
Tween is a registered trademark of ICI Americas, Inc.



Contents

Introduction.....	1
Applications	2
Materials Supplied	3
Required Equipment	4
Suitability	4
Device Storage	4
Specifications	5
Chemical Compatibility	7
How to Use Amicon Ultra-0.5 Centrifugal Filter Devices	9
How to Quantitate Recoveries	11
Direct Weighing Procedure	11
Performance - DNA Concentration	14
Performance - Protein Concentration	15
Flow Rate.....	15
Protein Retention and Concentrate Recovery.....	18
Maximizing Sample Recovery	21
Desalting or Diafiltration.....	22
Centrifugal Product Ordering Information	23
Technical Assistance	24
Standard Warranty.....	25

Introduction

Millipore's Amicon® Ultra-0.5 centrifugal filter devices provide **fast ultrafiltration**, with the capability for **high concentration factors** and **easy concentrate recovery from dilute and complex sample matrices**. The vertical design and available membrane surface area provide fast sample processing, **high sample recovery (typically greater than 90% of dilute starting solution)**, and the capability for **30-fold concentration**. **Typical processing time is 10 to 30 minutes** depending on Nominal Molecular Weight Limit (NMWL). **Solute polarization and subsequent fouling** of the membrane are **minimized** by the vertical design, and a **physical deadstop in the filter device prevents spinning to dryness** and potential sample loss. **Efficient recovery of the concentrated sample (retained species) is achieved by a convenient reverse spin step after collecting the filtrate**. Amicon Ultra-0.5 devices are supplied non-sterile and are for single use only.

Introduction, continued


The Amicon Ultra-0.5 product line includes 5 different cutoffs (Nominal Molecular Weight Limit, NMWL). These devices are for research use only and not for use in diagnostic procedures.

- Amicon Ultra 3K device — 3,000 NMWL
- Amicon Ultra 10K device — 10,000 NMWL
- Amicon Ultra 30K device — 30,000 NMWL
- Amicon Ultra 50K device — 50,000 NMWL
- Amicon Ultra 100K device — 100,000 NMWL

Applications

- Concentration of biological samples containing antigens, antibodies, enzymes, nucleic acids (DNA/RNA samples, either single- or double-stranded), microorganisms, column eluates, and purified samples
- Purification of macromolecular components found in tissue culture extracts and cell lysates, removal of primer, linkers, or molecular labels from a reaction mix, and protein removal prior to HPLC
- Desalting, buffer exchange, or diafiltration

Materials Supplied

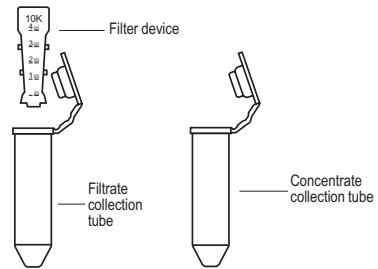

The Amicon Ultra-0.5 device is supplied with two microcentrifuge tubes. During operation, one tube is used to collect filtrate; the other to recover the concentrated sample.

Required Equipment

- Centrifuge with fixed angle rotor that can accommodate 1.5 mL microcentrifuge tubes

CAUTION: To avoid damage to the device during centrifugation, check clearance before spinning.

Suitability

Preliminary recovery and retention studies are suggested to ensure suitability for intended use. See the “How to Quantitate Recoveries” section.

Device Storage

Store at room temperature.

Specifications

Maximum initial sample volume	500 μ L
Typical final concentrate volume	15–20 μ L
Recommended relative centrifugal force	14,000 \times g for concentration spin 1,000 \times g for reverse spin
Maximum relative centrifugal force	15,000 \times g
Active membrane area	1 cm ²
Hold-up volume	< 5 μ L

Dimensions

Filter device and tube

Length (concentration mode; device in tube): 49.9 mm (1.96 in.)

Length (reverse spin; device upside down in tube): 47.4 mm (1.87 in.)

Tube (cap closed) Diameter: 10.8 mm (0.43 in.) Length: 42.1 mm (1.66 in.)

Filter device Diameter: 9.4 mm (0.37 in.) Length: 29.5 mm (1.16 in.)

Materials of Construction

Filter device	Copolymer styrene/butadiene
Membrane	Millipore Ultracel [®] low binding regenerated cellulose
Collection tube	Polypropylene

Specifications, continued

The ultrafiltration membranes in Amicon Ultra-0.5 devices contain trace amounts of the following:

- Amicon Ultra 3K devices: glycerine
- Amicon Ultra 10K device: triethylene glycol (TEG)
- Amicon Ultra 30K devices: glycerine
- Amicon Ultra 50K devices: glycerine
- Amicon Ultra 100K devices: glycerine

If these materials interfere with analysis, pre-rinse the device with buffer or Milli-Q® water. If interference continues, rinse with 0.1 N NaOH followed by a second spin of buffer or Milli-Q water.

CAUTION: Do not allow the membrane in Amicon Ultra filter devices to dry out once wet. If you are not using the device immediately after pre-rinsing, leave fluid on the membrane until the device is used.

Chemical Compatibility

Amicon Ultra centrifugal devices are intended for use with biological fluids and aqueous solutions. Before use, check the sample for chemical compatibility with the device.

Table 1. Chemical Compatibility of Amicon Ultra Filter Devices

Acids		Concentration		Concentration	
Acetic acid	≤ 50%*	Phosphoric acid	≤ 30%		
Formic acid	≤ 5%*	Sulfamic acid	≤ 3%		
Hydrochloric acid	≤ 1.0 M	Sulfuric acid	≤ 3%		
Lactic acid	≤ 50%	Trichloroacetic acid (TCA)	≤ 10%*		
Nitric acid	≤ 10%	Trifluoroacetic acid (TFA)	≤ 30%*		
Alkalis					
Ammonium hydroxide	≤ 10%	Sodium hydroxide	≤ 0.5 M		
Alcohols					
n-Butanol	≤ 70%	Isopropanol	≤ 70%		
Ethanol	≤ 70%	Methanol	≤ 60%		
Detergents					
Alconox® detergent	≤ 1%	Lubrol® PX detergent	≤ 0.1%		
CHAPS detergent	≤ 0.1%	Nonidet™ P-40 surfactant	≤ 2%		

* Contact with this chemical may cause materials to leach out of the component parts. Solvent blanks are recommended to determine whether leachables represent potential assay interferences.

Chemical Compatibility, continued

Detergents, continued	Concentration		Concentration
Sodium deoxycholate	≤ 5%	Triton® X-100 surfactant	≤ 0.1%
Sodium dodecyl sulfate (SDS)	≤ 0.1%	Tween® 20 surfactant	≤ 0.1%
Terg-A-Zyme® detergent	≤ 1%		

Organic solvents

Acetone	not recommended	Ethyl acetate	not recommended
Acetonitrile	≤ 20%	Formaldehyde	≤ 5%
Benzene	not recommended	Pyridine	not recommended
Carbon tetrachloride	not recommended	Tetrahydrofuran	not recommended
Chloroform	not recommended	Toluene	not recommended
Dimethyl sulfoxide (DMSO)	≤ 5%*		


Miscellaneous

Ammonium sulfate	Saturated	Phenol	≤ 1%
Diethyl pyrocarbonate	≤ 0.2%	Phosphate buffer (pH 8.2)	≤ 1 M
Dithiothreitol (DTT)	≤ 0.1 M	Polyethylene glycol	≤ 10%
Glycerine	≤ 70%	Sodium carbonate	≤ 20%
Guanidine HCl	≤ 6 M	Tris buffer (pH 8.2)	≤ 1 M
Imidazole	≤ 100 mM	Urea	≤ 8 M
Mercaptoethanol	≤ 0.1 M		

* Contact with this chemical may cause materials to leach out of the component parts. Solvent blanks are recommended to determine whether leachables represent potential assay interferences.

How to Use Amicon Ultra-0.5 Centrifugal Filter Devices


1. Insert the Amicon Ultra-0.5 device into one of the provided microcentrifuge tubes.
2. Add up to 500 μL of sample to the Amicon Ultra filter device and cap it.
3. Place capped filter device into the centrifuge rotor, aligning the cap strap toward the center of the rotor; counterbalance with a similar device.
4. Spin the device at $14,000 \times g$ for approximately 10–30 minutes depending on the NMWL of the device used. Refer to Figure 1 and table 3 for typical spin times.

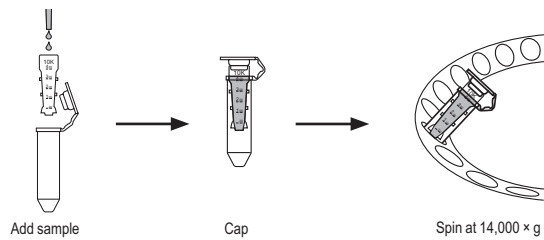

How to Use Amicon Ultra-0.5 Filter Devices, continued

5. Remove the assembled device from the centrifuge and separate the Amicon Ultra filter device from the microcentrifuge tube.
6. To recover the concentrated solute, place the Amicon Ultra filter device upside down in a clean micro centrifuge tube. Place in centrifuge, aligning open cap towards the center of the rotor; counterbalance with a similar device. Spin for 2 minutes at $1,000 \times g$ to transfer the concentrated sample from the device to the tube. The ultrafiltrate can be stored in the centrifuge tube.

NOTE: For optimal recovery, perform the reverse spin immediately.

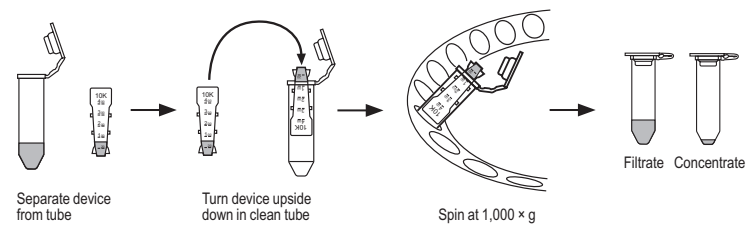

How to Quantitate Recoveries

Calculate total recovery, percent concentrate, and percent filtrate using the method below. The procedure provides a close approximation of recoveries for solutions having concentrations up to roughly 20 mg/mL.

NOTE: Appropriate assay techniques include absorption spectrophotometry, refractive index, and conductivity.

Direct Weighing Procedure

The density of most dilute proteins is nearly equal to the density of water (i.e., 1 g/mL). Using this property, the concentrate and filtrate recoveries can be quantitated by weighing them and converting the units from grams to milliliters. This technique is valid only for solutions with concentrations of approximately 20 mg/mL or less.

1. Separately weigh the empty filter device, filtrate collection tube, and concentrate collection tube before use.
2. Fill filter device with solution and reweigh.
3. Assemble device in filtrate collection tube and centrifuge per instructions.

Direct Weighing Procedure, continued

4. Collect the concentrate by reverse spin into the pre-weighed concentrate collection tube.
5. Remove the device from the concentrate collection tube and weigh the filtrate and concentrate collection tubes.
6. Subtract weight of empty device/tubes to calculate weights of starting material, filtrate, and concentrate.
7. Assay the filtrate and concentrate to determine solute concentration.
8. Calculate recoveries using the weight/volume data and the measured concentrations as follows:

$$\% \text{ concentrate recovery} = 100 \times \frac{W_c \times C_c}{W_o \times C_o}$$

$$\% \text{ filtrate recovery} = 100 \times \frac{W_f \times C_f}{W_o \times C_o}$$

$$\% \text{ total recovery} = \% \text{ concentrate recovery} + \% \text{ filtrate recovery}$$

Direct Weighing Procedure, continued

W_c = total weight of concentrate before assay

W_o = weight of original starting material

W_f = weight of filtrate

C_c = concentrate concentration

C_o = original starting material concentration

C_f = filtrate concentration

Performance - DNA Concentration

The Amicon Ultra-0.5 30K device provides the best balance between recovery and spin time for double-stranded DNA for base pairs ranging from 137 to 1159. To achieve maximum PCR product recovery and primer removal with primers greater than 20 bases, one or two additional spins with Tris-EDTA (TE) buffer are recommended.

Table 2. Typical recovery of nucleotides from Amicon Ultra-0.5 30K device

PCR Product (base pairs)	PCR Primer (bases)	PCR Recovery (%)	PCR Primer Removal (%)	TE Washes (number)
137	10	≥ 95	≥ 90	0
	20	≥ 90	≥ 85	1
	48	≥ 90	≥ 75	2
301	10	≥ 90	≥ 90	0
	20	≥ 85	≥ 90	1
	48	≥ 90	≥ 80	2
648	10	≥ 95	≥ 90	0
	20	≥ 90	≥ 90	1
	48	≥ 95	≥ 90	2
1159	10	≥ 90	≥ 90	0
	20	≥ 90	≥ 95	1
	48	≥ 95	≥ 95	2

Spin conditions: 40° fixed angle rotor, 14,000 × g, room temperature, 500 μL starting volume, 20–30 μL final volume, 10 minute spin, n=12.

Performance - Protein Concentration


Flow Rate

Factors affecting flow rate include sample concentration, starting volume, chemical nature of solute, relative centrifugal force, centrifuge rotor angle, membrane type, and temperature.

Figure 1 and Table 3 can be used to estimate the time required to achieve a given volume of filtrate or concentrate for a variety of protein markers. A typical spin time for a 500 μL sample in a fixed angle rotor is approximately 10–30 minutes (depending on device nominal molecular weight limit). While most of the sample is filtered in the first 5 to 10 minutes of centrifugation, the lowest concentrate volume (15–20 μL) is reached after spinning for 10–30 minutes.

Flow rate, continued

Figure 1. Typical Filtrate Volume vs. Spin Time

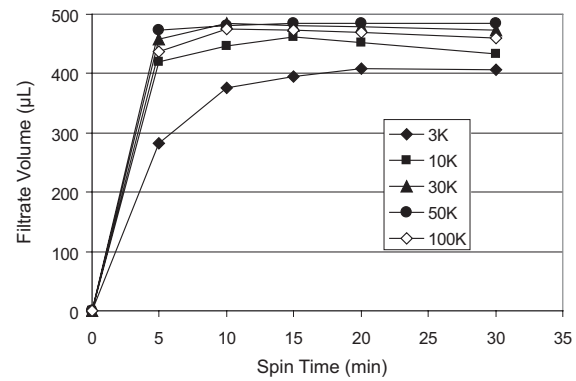

Spin conditions: 40° fixed angle rotor, 14,000 × g, room temperature, 500 µL starting volume.
Protein markers used: Cytochrome c for 3K and 10K, BSA for 30K and 50K, and IgG for 100K, n=8.

Flow rate, continued

Table 3. Typical Concentrate Volume / Concentration Factor vs. Spin Time

Spin time (min)	Concentrate volume / Concentration Factor									
	3K device		10K device		30K device		50K device		100K device	
	Conc. Volume (μ L)	Conc. Factor (x)	Conc. Volume (μ L)	Conc. Factor (x)	Conc. Volume (μ L)	Conc. Factor (x)	Conc. Volume (μ L)	Conc. Factor (x)	Conc. Volume (μ L)	Conc. Factor (x)
5	215	2	66	7	42	12	28	18	58	9
10	114	4	35	14	23	22	20	25	19	26
15	80	6	22	22	19	27	17	30	15	33
20	62	8	20	24	17	30	15	33	13	36
30	48	10	15	31	15	32	15	36	11	41

Spin conditions: 40° fixed angle rotor, 14,000 \times g, room temperature, 500 μ L starting volume. Protein markers used: Cytochrome c for 3K and 10K, BSA for 30K and 50K, and IgG for 100K, n=12. Shaded volumes were used for the calculation of protein recovery in Table 4.

Protein Retention and Concentrate Recovery

The membranes used in Amicon Ultra devices are characterized by a nominal molecular weight limit (NMWL); that is, their ability to retain molecules above a specified molecular weight. Solutes with molecular weights close to the NMWL may be only partially retained. Membrane retention depends on the solute's molecular size and shape. For most applications, molecular weight is a convenient parameter to use in assessing retention characteristics. Millipore recommends using a membrane with a NMWL at least two times smaller than the molecular weight of the protein solute that one intends to concentrate. Refer to Table 4 for "Typical Retention of Protein Markers".

Protein Retention and Concentrate Recovery, continued

Table 4: Typical Retention of Protein Markers

Marker/Concentration	Molecular Weight	Device NMWL	% Retention	Spin Time (min)
α -Chymotrypsinogen (1 mg/mL)	25,000	3K	> 95	30
Cytochrome c (0.25 mg/mL)	12,400		> 95	30
Vitamin B-12 (0.2 mg/mL)	1,350		< 42	30
α -Chymotrypsinogen (1 mg/mL)	25,000	10K	> 95	15
Cytochrome c (0.25 mg/mL)	12,400		> 95	15
Vitamin B-12 (0.2 mg/mL)	1,350		< 42	15
BSA (1 mg/mL)	67,000	30K	> 95	10
Ovalbumin (1 mg/mL)	45,000		> 95	10
Cytochrome c (0.25 mg/mL)	12,400		< 35	10
BSA (1 mg/mL)	67,000	50K	> 95	10
Ovalbumin (1 mg/mL)	45,000		~ 40	10
Cytochrome c (0.25 mg/mL)	12,400		< 20	10
Thyroglobulin (0.5 mg/mL)	677,000	100K	> 95	10
IgG (1 mg/mL)	156,000		> 95	10
Ovalbumin (1 mg/mL)	45,000		< 30	10

Spin Conditions: 40° fixed angle rotor, 14,000 × g, room temperature, 500 μ L starting volume, n=12.

Protein Retention and Concentrate Recovery, continued

Factors that determine sample recovery include the nature of the protein solute relative to the device NMWL chosen, starting concentration, and concentration factor. Table 5 provides typical recoveries for Amicon Ultra-0.5 devices.

Table 5. Typical Concentrate Recovery

Marker/ Concentration	Molecular Weight	Device NMWL	Spin Time (min)	Concentrate Volume (µL)	Concentration Factor (x)	Concentrate Recovery (%)
Cytochrome c (0.25 mg/mL)	12,400	3K	30	48	10	98
Cytochrome c (0.25 mg/mL)	12,400	10K	15	22	22	93
BSA (1 mg/mL)	67,000	30K	10	23	22	97
BSA (1 mg/mL)	67,000	50K	10	20	25	92
IgG (1 mg/mL)	156,000	100K	10	19	26	92

Spin Conditions: 40° fixed angle rotor, 14,000 × g, room temperature, 500 µL starting volume, n=12.
The shaded volumes were taken from Table 3.


Maximizing Sample Recovery

Low sample recovery in the concentrate may be due to adsorptive losses, over-concentration, or passage of sample through the membrane.

- Adsorptive losses depend upon solute concentration, its hydrophobic nature, temperature and time of contact with filter device surfaces, sample composition, and pH. To minimize losses, remove concentrated samples immediately after centrifugal spin.
- If starting sample concentration is high, monitor the centrifugation process in order to avoid over-concentration of the sample. Over-concentration can lead to precipitation and potential sample loss.
- If the sample appears to be passing through the membrane, choose a lower NMWL Amicon Ultra-0.5 device.

Desalting or Diafiltration

Desalting, buffer exchange, or diafiltration are important methods for removing salts or solvents in solutions containing biomolecules. The removal of salts or the exchange of buffers can be accomplished in the Amicon Ultra-0.5 device by concentrating the sample, then reconstituting the concentrate to the original sample volume with any desired solvent. The process of "washing out" can be repeated until the concentration of the contaminating microsolite has been sufficiently reduced. See example below.

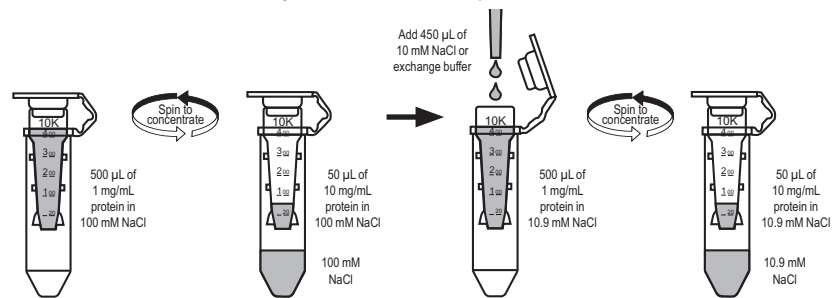

Centrifugal Product Ordering Information

Initial volume (mL)	Final concentrate volume (µL)	Product	Qty / pk	3,000 NMWL	10,000 NMWL	30,000 NMWL	50,000 NMWL	100,000 NMWL
0.5	20	Amicon Ultra-0.5 device	8	UFC500308	UFC501008	UFC503008	UFC505008	UFC510008
			24	UFC500324	UFC501024	UFC503024	UFC505024	UFC510024
			96	UFC500396	UFC501096	UFC503096	UFC505096	UFC510096
			500	UFC5003BK	UFC5010BK	UFC5030BK	UFC5050BK	UFC5100BK
Amicon Ultra-0.5 Collection Tubes			96	UFC50VL96				
4	30–70	Amicon Ultra-4 device	8	UFC800308	UFC801008*	UFC803008	UFC805008	UFC810008
			24	UFC800324	UFC801024*	UFC803024	UFC805024	UFC810024
			96	UFC800396	UFC801096*	UFC803096	UFC805096	UFC810096
15	150–300	Amicon Ultra-15 device	8	UFC900308	UFC901008*	UFC903008	UFC905008	UFC910008
			24	UFC900324	UFC901024*	UFC903024	UFC905024	UFC910024
			96	UFC900396	UFC901096*	UFC903096	UFC905096	UFC910096

Related Products

* Amicon Ultra-4 and -15 10,000 NMWL devices are for in vitro diagnostic use. All other devices are for research use only.

70	350	Centricron® Plus-70 device	8	UFC700508	UFC701008	UFC703008	N/A	UFC710008
0.5	20	MultiScreen® 96 well plate/ Ultracel-10 membrane	10	N/A	MAUF01010	N/A	N/A	N/A

Technical Assistance

For more information, contact the Millipore office nearest you. In the U.S., call **1-800-MILLIPORE** (1-800-645-5476). Outside the U.S., see your Millipore catalogue for the phone number of the office nearest you or go to our web site at www.millipore.com/offices for up-to-date worldwide contact information. You can also visit the tech service page on our web site at www.millipore.com/techservice.

Standard Warranty

Millipore Corporation ("Millipore") warrants its products will meet their applicable published specifications when used in accordance with their applicable instructions for a period of one year from shipment of the products. **MILLIPORE MAKES NO OTHER WARRANTY, EXPRESSED OR IMPLIED. THERE IS NO WARRANTY OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE.** The warranty provided herein and the data, specifications, and descriptions of Millipore products appearing in Millipore's published catalogues and product literature may not be altered except by express written agreement signed by an officer of Millipore. Representations, oral or written, which are inconsistent with this warranty or such publications are not authorized and if given, should not be relied upon.

In the event of a breach of the foregoing warranty, Millipore's sole obligation shall be to repair or replace, at its option, the applicable product or part thereof, provided the customer notifies Millipore promptly of any such breach. If after exercising reasonable efforts, Millipore is unable to repair or replace the product or part, then Millipore shall refund to the customer all monies paid for such applicable product or part. **MILLIPORE SHALL NOT BE LIABLE FOR CONSEQUENTIAL, INCIDENTAL, SPECIAL, OR ANY OTHER INDIRECT DAMAGES RESULTING FROM ECONOMIC LOSS OR PROPERTY DAMAGE SUSTAINED BY ANY CUSTOMER FROM THE USE OF ITS PRODUCTS.**

